


Ambulatory Patient Suggested Modality Quick Reference Guide

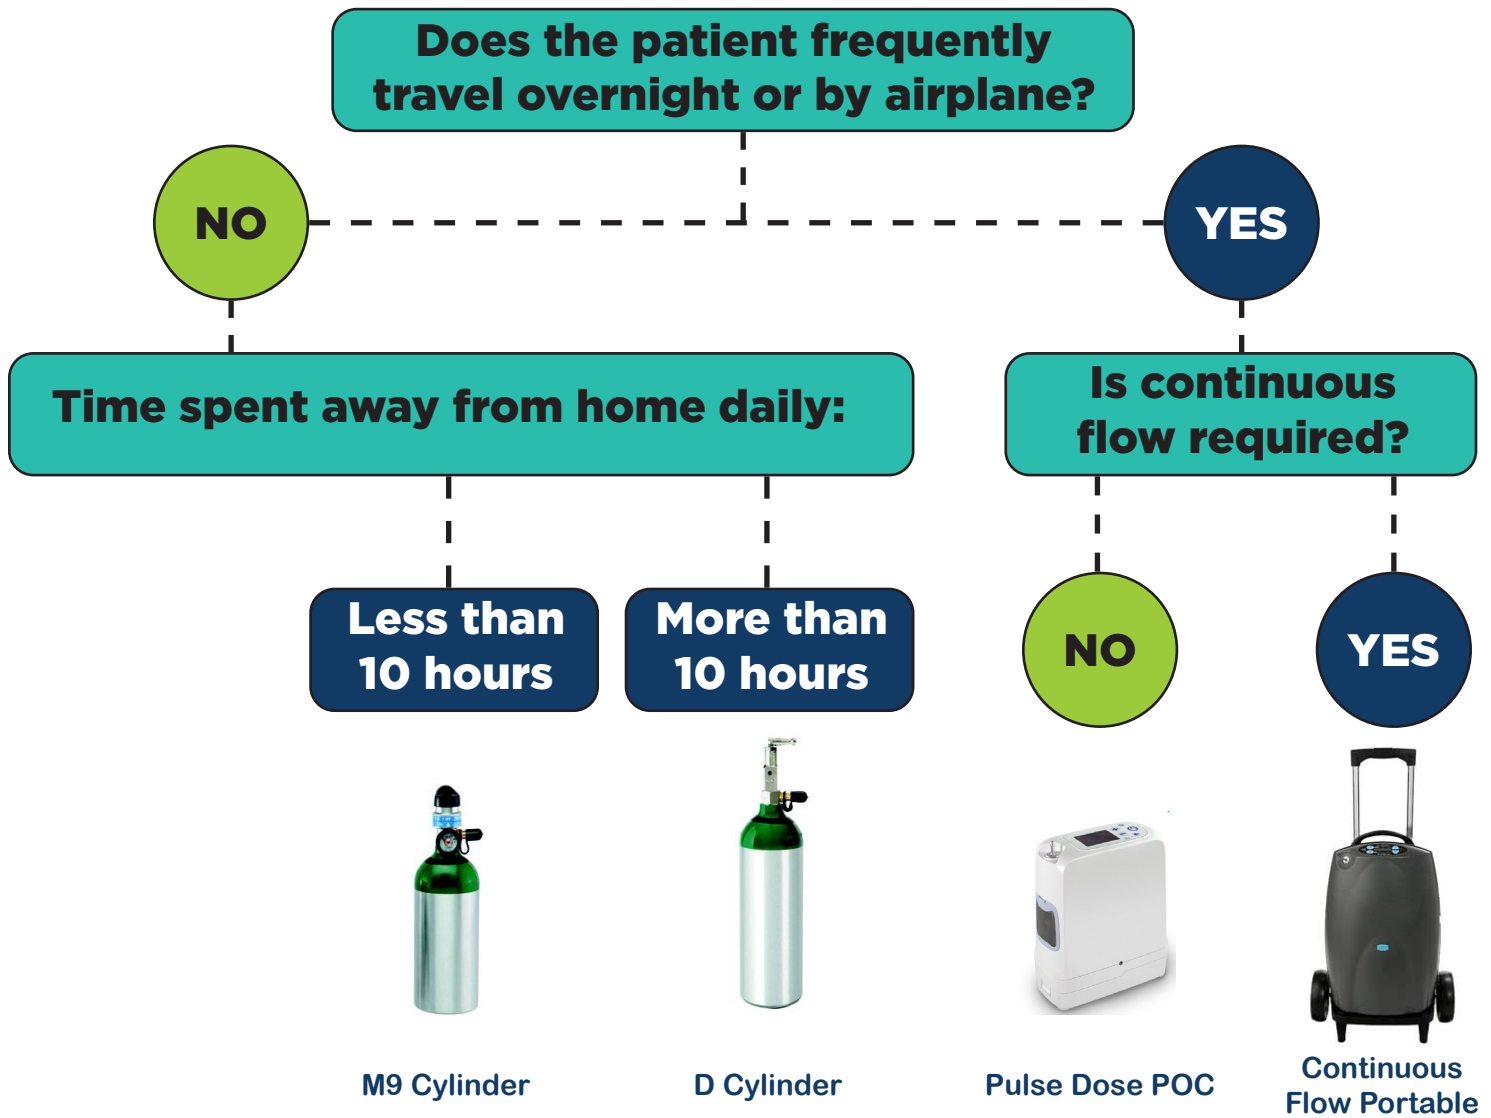

Duration on Pulse Setting 2	10.1 hrs.*	depends on conservor used	5 hrs.	5.1 hrs
Duration on Continuous Flow 2	2.3 hrs.	3.5 hrs.	N/A	2 hrs.
Weight	5.1 lbs.	6.3 lbs.	4.74 lbs.	18.4 lbs.

*Duration calculated for 20 breaths/minute using nominal pulse volume.

For additional information, contact your React Health representative or visit reacthealth.com

The information provided in this document is intended only to be general in nature, does not represent or constitute medical advice, and is not intended to influence or replace a healthcare provider's independent assessment and care of any patient, based on a patient's individual context and health status. Each patient should be examined and advised individually by a licensed healthcare professional. For product use and operation always consult and follow all applicable user manuals, safety information, product inserts, and instructions for use.