

SD Card Compliance Report for John Doe

Date generated: 06/18/2021


Patient Information	Provider Information	Physician Information
Patient name: John Doe	Organization:	Name:
Patient ID:	Address 1:	Organization:
Device serial: ES421123456	Address 2:	Address 1:
Gender: Male	Country:	Address 2:
Date of birth:	City:	Country:
Therapy start:	State:	City:
Address 1:	ZIP code:	State:
Address 2:	Phone:	ZIP code:
Country:		Phone:
City:		
State:		
ZIP code:		

Device Settings

Mode	Auto-CPAP
Ramp pressure	4.0 cmH2O
Minimum pressure	9.0 cmH2O
Maximum pressure	20.0 cmH2O

Compliance Summary

Start date	01/28/2021
End date	02/26/2021
Days in range	30
Days of use	30 / 30 days (100.0%)
Total usage in date range	6 days, 8 hours, 41 minutes
Average usage (on days used)	5 hours, 5 minutes
Average usage (on all days)	5 hours, 5 minutes
Maximum usage	7 hours, 2 minutes
Minimum usage	2 hours, 28 minutes
Days with usage >= 4 hours	86.7% (26 of 30 days)

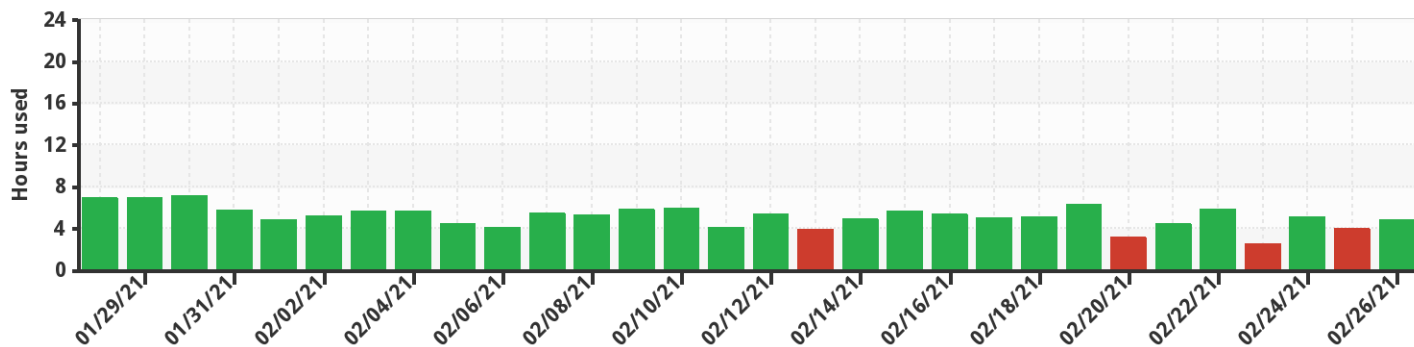

Usage Summary

Mean pressure	7.9 cmH2O
Average P95	10.6 cmH2O
Highest daily average pressure	9.5 cmH2O
Lowest daily average pressure	6.0 cmH2O
Average high leak time	0 minutes
Average leak	0.5 LPM
Average AHI	4.3
Average CAI	1.2

Key


P95: device was at or under this pressure 95% of the time

High leak time: amount of time spent blowing with a leak > 90 L/min.


CAI: clear airway apnea index

Clinical Summary


AHI and CAI

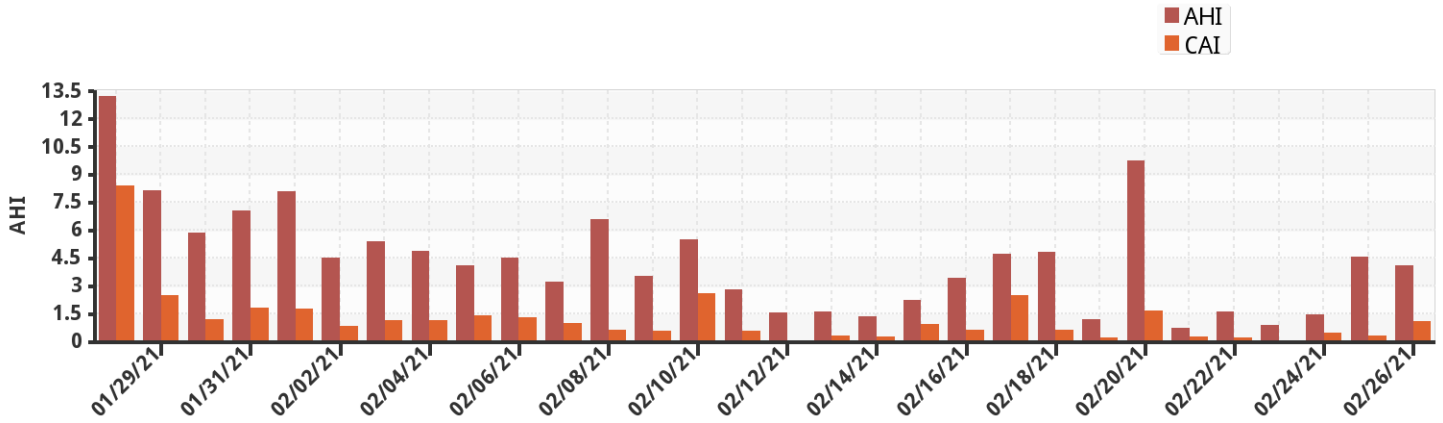

Average leak

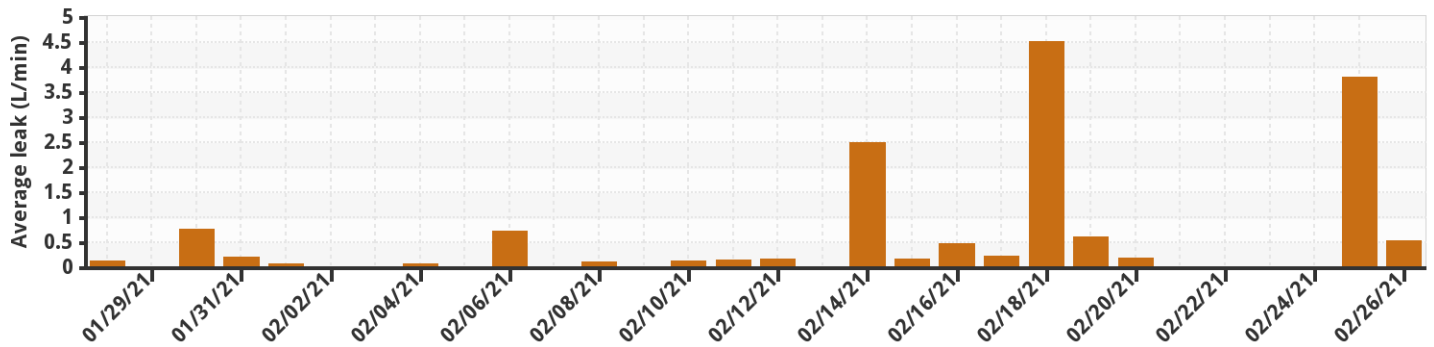

Average pressure, P95, and maximum pressure

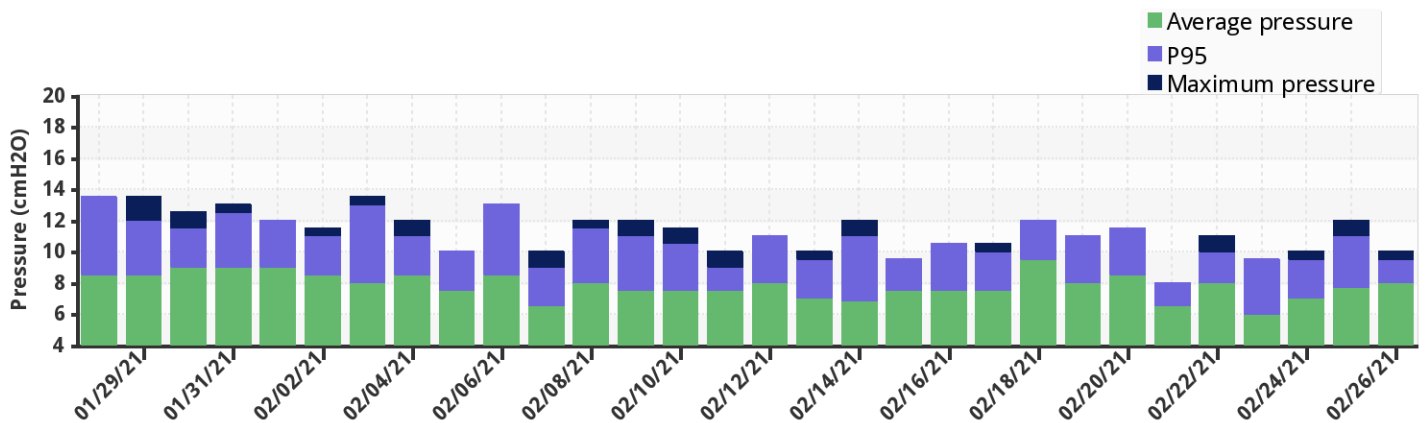

Daily usage

Date	Use time (hh:mm)	P95	Average pressure	CAI	AHI	Apnea count	Hypopnea count	Average leak	High leak (>90 LPM) (hh:mm)
02/26/2021	04:43	9.0 cmH2O	8.0 cmH2O	1.1	4	10	4	0.5 LPM	00:00
02/25/2021	03:55	11.0 cmH2O	7.7 cmH2O	0.3	4.5	14	2	3.8 LPM	00:04
02/24/2021	05:03	9.0 cmH2O	7.0 cmH2O	0.4	1.4	3	2	0.0 LPM	00:00
02/23/2021	02:28	9.0 cmH2O	6.0 cmH2O	0	0.8	2	0	0.0 LPM	00:00
02/22/2021	05:44	10.0 cmH2O	8.0 cmH2O	0.2	1.6	5	3	0.0 LPM	00:00
02/21/2021	04:22	8.0 cmH2O	6.5 cmH2O	0.2	0.7	0	2	0.0 LPM	00:00
02/20/2021	03:05	11.0 cmH2O	8.5 cmH2O	1.6	9.7	19	6	0.2 LPM	00:00
02/19/2021	06:15	11.0 cmH2O	8.0 cmH2O	0.2	1.1	2	4	0.6 LPM	00:00
02/18/2021	05:02	12.0 cmH2O	9.5 cmH2O	0.6	4.8	14	7	4.5 LPM	00:00
02/17/2021	04:56	10.0 cmH2O	7.5 cmH2O	2.4	4.7	9	2	0.2 LPM	00:00
02/16/2021	05:18	10.0 cmH2O	7.5 cmH2O	0.6	3.4	8	7	0.5 LPM	00:00
02/15/2021	05:33	9.0 cmH2O	7.5 cmH2O	0.9	2.2	2	5	0.2 LPM	00:00
02/14/2021	04:49	11.0 cmH2O	6.9 cmH2O	0.2	1.3	4	1	2.5 LPM	00:07
02/13/2021	03:51	9.0 cmH2O	7.0 cmH2O	0.3	1.6	3	2	0.0 LPM	00:00
02/12/2021	05:20	11.0 cmH2O	8.0 cmH2O	0	1.5	8	0	0.2 LPM	00:00
02/11/2021	04:01	9.0 cmH2O	7.5 cmH2O	0.5	2.7	6	3	0.1 LPM	00:00
02/10/2021	05:51	10.0 cmH2O	7.5 cmH2O	2.6	5.5	9	8	0.1 LPM	00:00
02/09/2021	05:44	11.0 cmH2O	7.5 cmH2O	0.5	3.5	11	6	0.0 LPM	00:00
02/08/2021	05:13	11.0 cmH2O	8.0 cmH2O	0.6	6.5	23	8	0.1 LPM	00:00
02/07/2021	05:24	9.0 cmH2O	6.5 cmH2O	0.9	3.1	7	5	0.0 LPM	00:00
02/06/2021	04:03	13.0 cmH2O	8.5 cmH2O	1.2	4.4	7	6	0.7 LPM	00:00
02/05/2021	04:25	10.0 cmH2O	7.5 cmH2O	1.4	4.1	10	2	0.0 LPM	00:00
02/04/2021	05:36	11.0 cmH2O	8.5 cmH2O	1.1	4.8	15	6	0.1 LPM	00:00
02/03/2021	05:37	13.0 cmH2O	8.0 cmH2O	1.1	5.3	18	6	0.0 LPM	00:00
02/02/2021	05:10	11.0 cmH2O	8.5 cmH2O	0.8	4.5	11	8	0.0 LPM	00:00
02/01/2021	04:44	12.0 cmH2O	9.0 cmH2O	1.7	8	18	12	0.1 LPM	00:00
01/31/2021	05:42	12.0 cmH2O	9.0 cmH2O	1.8	7	20	10	0.2 LPM	00:00
01/30/2021	07:02	11.0 cmH2O	9.0 cmH2O	1.1	5.8	19	14	0.8 LPM	00:00
01/29/2021	06:55	12.0 cmH2O	8.5 cmH2O	2.5	8.1	25	14	0.0 LPM	00:00
01/28/2021	06:50	13.0 cmH2O	8.5 cmH2O	8.3	13.2	24	9	0.1 LPM	00:00